

PRIOR ART

FIG. 1

FIG. 2 is a perspective view of the device 100 in a first position.

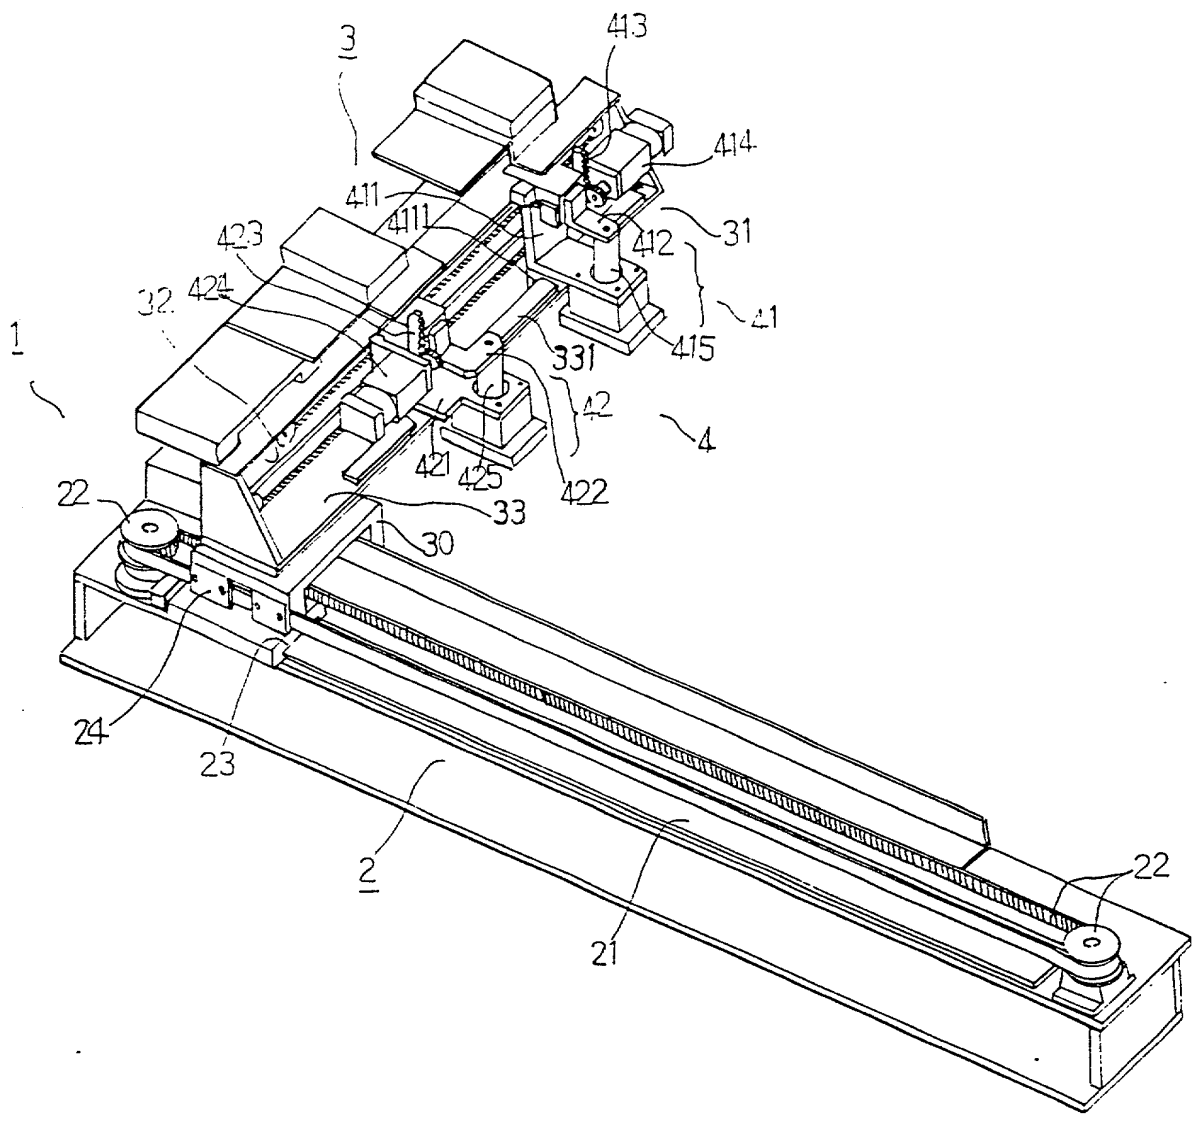


FIG. 2

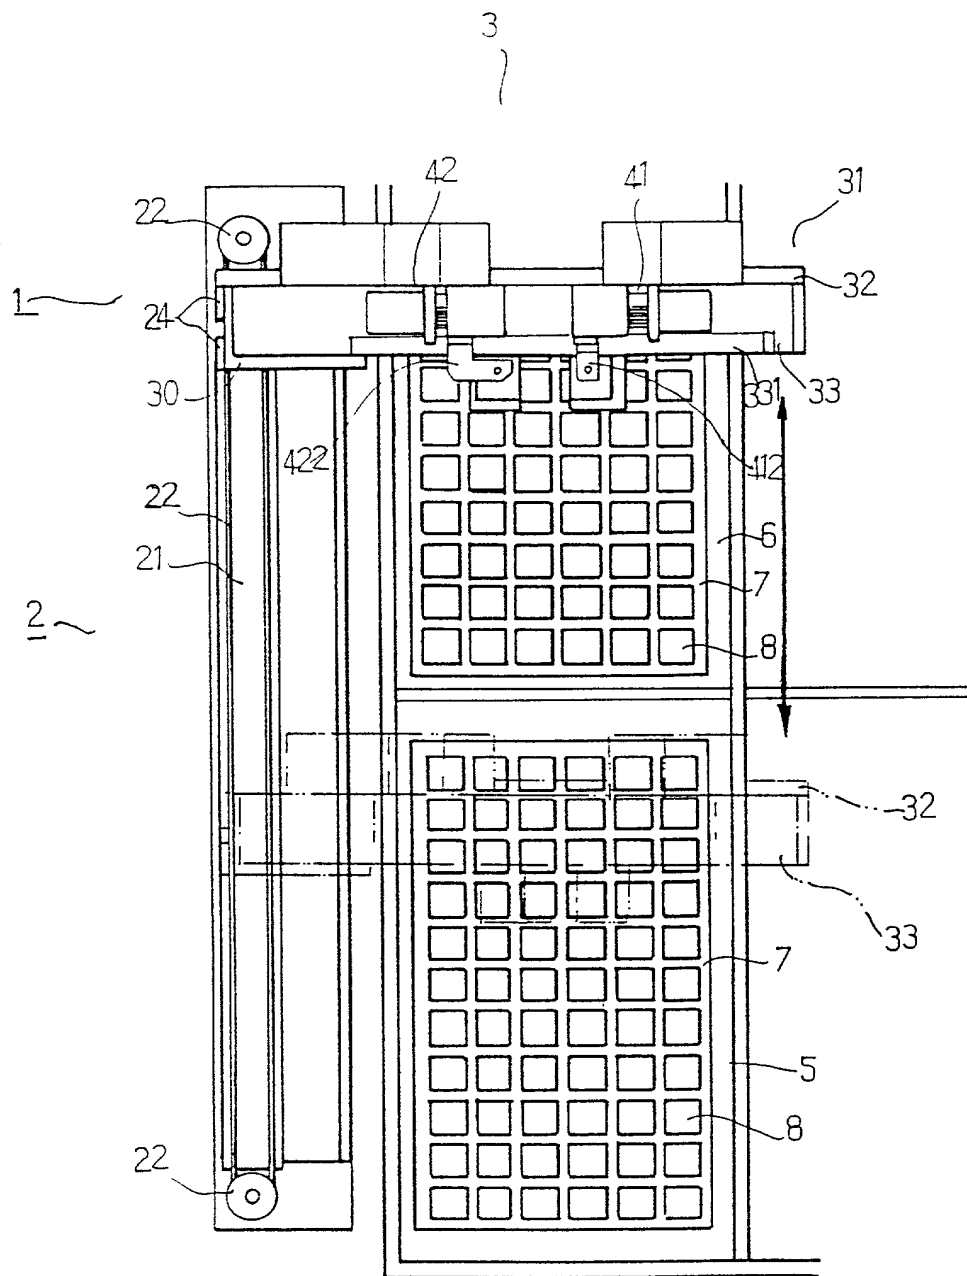


FIG. 3

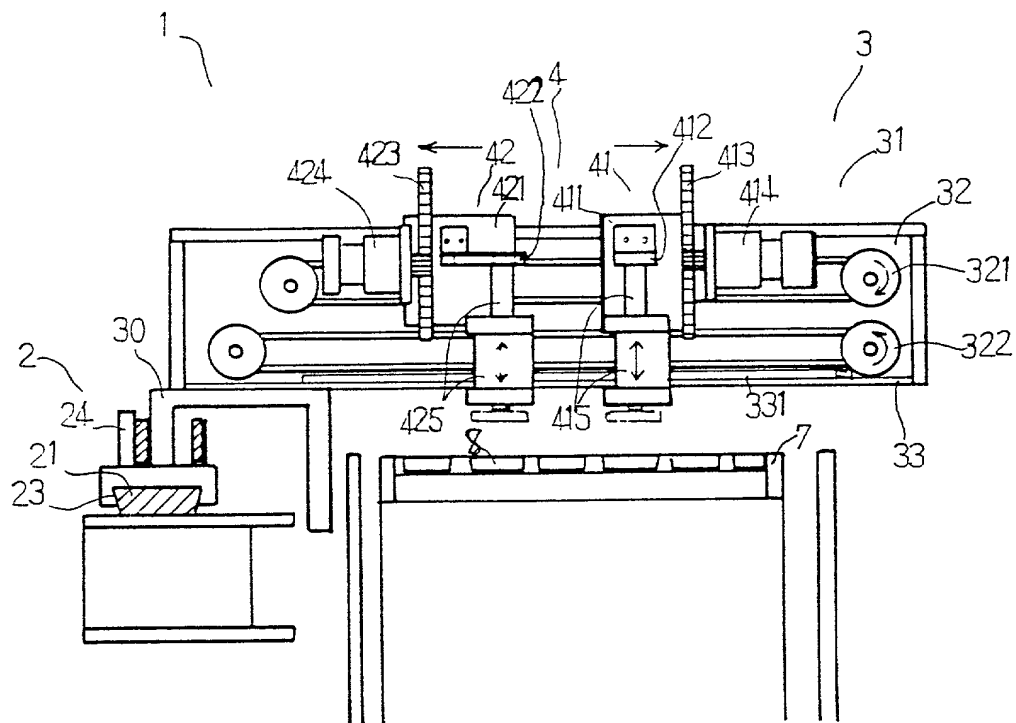


FIG. 4